


Q2. Which instrument should be selected?

A2. Recommended usage order for non-biohazardous samples.

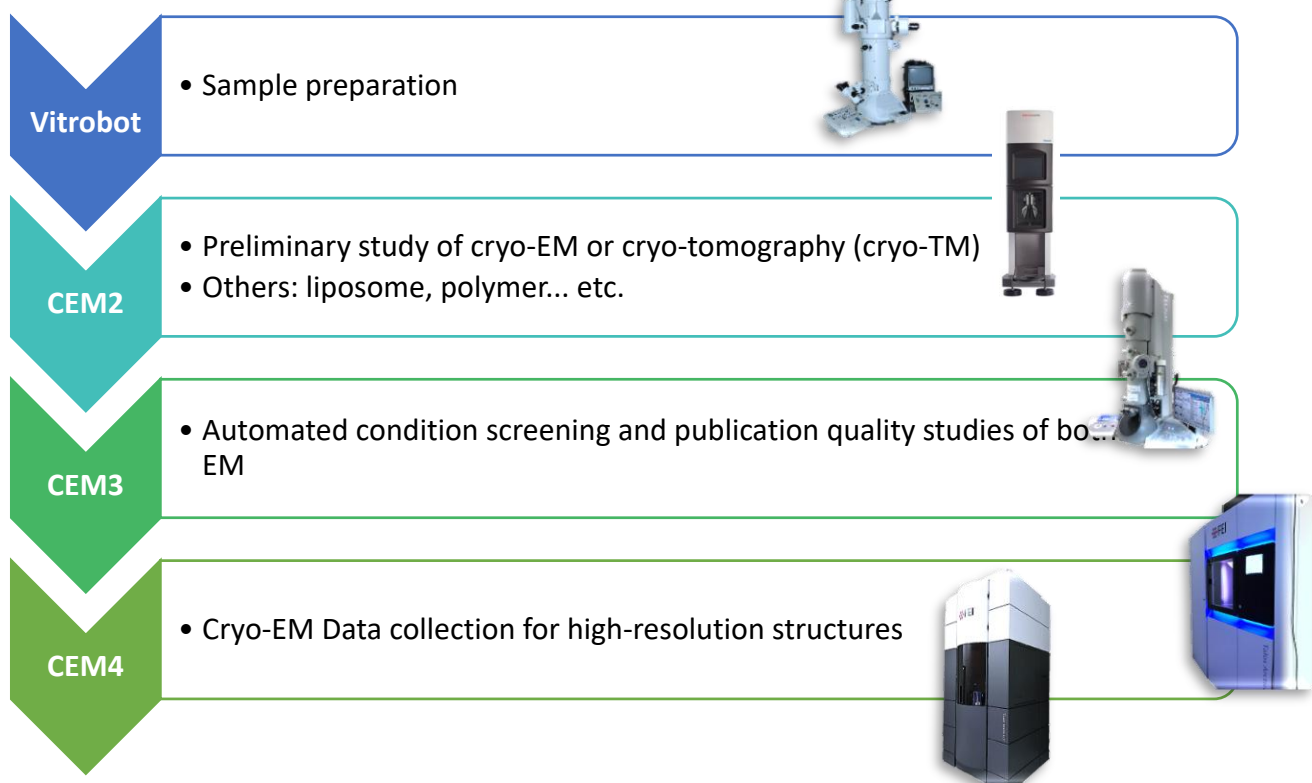

For consultation, please contact us via cryoem@gate.sinica.edu.tw .